

Orange, Sam, Metcalfe, James W.,
Liefieith, Andreas ORCID: <https://orcid.org/0000-0003-2121-3219>,
Marshall, Phil, Madden, Leigh A., Fewster, Connor R. and Vince,
Rebecca V. (2018) Validity and Reliability of a Wearable Inertial
Sensor to Measure Velocity and Power in the Back Squat and
Bench Press. Journal of Strength and Conditioning Research.

Downloaded from: <http://ray.yorks.ac.uk/id/eprint/3118/>

The version presented here may differ from the published version or version of record. If
you intend to cite from the work you are advised to consult the publisher's version:
<https://doi.org/10.1519/JSC.0000000000002574>

Research at York St John (RaY) is an institutional repository. It supports the principles of
open access by making the research outputs of the University available in digital form.
Copyright of the items stored in RaY reside with the authors and/or other copyright
owners. Users may access full text items free of charge, and may download a copy for
private study or non-commercial research. For further reuse terms, see licence terms
governing individual outputs. [Institutional Repository Policy Statement](#)

RaY

Research at the University of York St John

For more information please contact RaY at ray@yorks.ac.uk

Validity and Reliability of a Wearable Inertial Sensor to Measure Velocity and Power in the Back Squat and Bench Press

Samuel T. Orange^{1,2*}, James W. Metcalfe^{1,2}, Andreas Liefeth², Phil Marshall¹, Leigh A. Madden³, Connor R. Fewster⁴ and Rebecca V. Vince¹.

¹Sport, Health and Exercise Science, School of Life Sciences, University of Hull, Hull, UK.

²School of Sport, York St John University, York, UK.

³Centre of Biomedical Research, School of Life Sciences, University of Hull, Hull, UK.

⁴Carnegie School of Sport, Leeds Beckett University, Leeds, UK.

*Corresponding author

Samuel T. Orange

¹Sport, Health and Exercise Science, School of Life Sciences

University of Hull, Cottingham Road, Hull, UK, HU6 7RX.

Email: orange_1@hotmail.co.uk

Telephone: +44 (0)1482 466314

Brief running head: Validity and reliability of an inertial sensor

Disclosure statement: This research did not receive any specific grant from funding agencies in the public, commercial, or not-for-profit sectors.

ABSTRACT

This study examined the validity and reliability of a wearable inertial sensor to measure velocity and power in the free-weight back squat and bench press. Twenty-nine youth rugby league players (18 ± 1 years) completed two test-retest sessions for the back squat followed by two test-retest sessions for the bench press. Repetitions were performed at 20%, 40%, 60%, 80% and 90% of one repetition maximum (1RM) with mean velocity (MV), peak velocity (PV), mean power (MP) and peak power (PP) simultaneously measured using an inertial sensor (PUSHTM) and a linear position transducer (GymAware PowerTool). PUSHTM only demonstrated good validity (Pearson product-moment correlation coefficient [r]) and reliability (intraclass correlation coefficient [ICC]) for measurements of MP ($r = 0.91$; ICC = 0.83) and PP ($r = 0.90$; ICC = 0.80) at 20% of 1RM in the back squat. However, it may be more appropriate for athletes to jump off the ground with this load to optimise power output. Further research should therefore evaluate the usability of inertial sensors in the jump squat exercise. In the bench press, good validity and reliability were only evident for the measurement of MP at 40% of 1RM ($r = 0.89$; ICC = 0.83). PUSHTM was unable to provide a valid and reliable estimate of any other criterion variable in either exercise. Practitioners must be cognisant of the measurement error when using inertial sensor technology to quantify velocity and power during resistance training, particularly with loads other than 20% of 1RM in the back squat and 40% of 1RM in the bench press.

Key words: Linear position transducer, rugby league, sports performance, strength and conditioning.

INTRODUCTION

The use of velocity-based feedback has recently emerged as an effective strategy to monitor loading intensity (10, 17) and estimate the proximity of repetition failure (29) during resistance training. A progressive decline in repetition velocity is also representative of acute neuromuscular fatigue during isoinertial loading (33). Furthermore, objectively measuring mechanical power during resistance training enables the strength and conditioning (S&C) practitioner to determine the load that elicits optimal power output and quantify training-induced adaptations (40). The accurate measurement of velocity and power is contingent on the development of valid and reliable instruments that are usable in the field (2).

Force platforms are widely considered the gold standard for the direct acquisition of kinetic data (14). This technique may be less appropriate for measuring barbell velocity, however, because force platforms are unable to account for barbell movements that occur independent of the body (12). In addition, force platforms are generally not available for use within a practical setting (11). Linear position transducers (LPTs) are portable kinematic systems that directly measure the vertical displacement of a cable (that is attached to the barbell) and determine velocity and power through double differentiation processes (12). GymAware PowerTool (GYM) is a commercially available LPT that provides immediate kinematic feedback and automated summary reports on a cloud-based system. GYM has recently been shown to accurately assess velocity and power output in the free-weight back squat (6) and bench press (15) compared to laboratory-based criterion measures. However, the relatively high monetary cost of GYM (~£1700 per unit) limits its widespread application to all sporting organisations. The requirement of a cable attachment to the barbell also restricts the number of resistance exercises it can accurately measure. This has given rise to the increased popularity of various wearable devices to improve the accessibility of tracking kinematic and kinetic variables during resistance training.

67 A wearable inertial sensor has recently been developed (PUSHTM) to quantify movement
68 velocity and power output in resistance training exercises. The device is relative economical
69 (~£220 per unit) and is worn inconspicuously on the forearm. Good correlations between
70 PUSHTM and a LPT have previously been reported for the measurement of mean and peak
71 velocity in the Smith machine back squat (5). Sato et al. (35) also suggested that PUSHTM is
72 highly valid at measuring movement velocity in the dumbbell biceps curl and dumbbell
73 shoulder press. However, the Pearson correlation analyses employed in both studies (5, 35)
74 involved combining all repetitions performed by each individual. That is, all participants
75 provided multiple data points in each paired measure. This statistical technique, although a
76 widespread practice, violates the assumption of independence of error between observations in
77 the Pearson correlation analysis (4). Analysing non-independent data with techniques that
78 assume independence often produces specious results (1, 26). Combining all repetitions for
79 analysis also does not elucidate whether the validity of the inertial sensor is load dependent.

80 In the only other study evaluating the validity of PUSHTM to date, Banyard and colleagues (6)
81 compared PUSHTM to a laboratory-based testing device in the free-weight back squat. Ten
82 resistance-trained males lifted loads of 20, 40, 60, 80, 90 and 100% of one repetition maximum
83 (1RM), with the fastest repetition from each load used for correlation analysis. Their results
84 suggested that the validity of PUSHTM to assess velocity and power in the back squat was
85 questionable (6). Although the data were appropriately analysed and provide useful
86 information, the applicability of these results to athlete populations is somewhat limited
87 because the study involved a small sample of recreationally-trained men. Athletic populations
88 require sessional and weekly training loads to be monitored with increased precision because
89 of a typically greater training burden and the need to prepare for competition. Within-subject
90 variation is also likely to differ between athlete and recreational populations (21). To determine

the usability of PUSHTM within professional sport, it is essential to evaluate its validity in a larger sample of professional athletes.

Despite receiving considerable academic and practitioner interest in recent years, the test-retest reliability of the PUSHTM device is yet to be determined. Previous studies have either not employed a repeated measures design that permits a test-retest analysis (5, 35) and/or have not reported any reliability statistics (6, 35). Similarly, the smallest difference between repeated trials that is not due to measurement error or variation within individual performance, termed the smallest worthwhile change (SWC) (22), has not been established. Therefore, the purpose of this study was to evaluate the concurrent validity and test-retest reliability of a wearable inertial sensor to measure velocity and power output during the free-weight back squat and bench press in professional youth rugby league players.

METHODS

Experimental Approach to the Problem

Using a repeated measures design, participants visited the laboratory on five separate occasions. The first visit was a familiarisation session where 1RMs were determined for the free-weight back squat and bench press. Participants were also familiarised with executing the concentric phase of each repetition with maximal intentional velocity. Visits two and three to the laboratory involved test and retest sessions for the back squat, whereas visits four and five were test and retest sessions for the bench press. Each of these testing sessions involved the completion of repetitions at 20%, 40%, 60%, 80% and 90% of 1RM. Mean velocity (MV), peak velocity (PV), mean power (MP) and peak power (PP) of each repetition were simultaneously recorded using a commercially available LPT (GymAware PowerTool [GYM], Kinetic Performance Technologies, Canberra, Australia) and a wearable inertial sensor

(PUSH™, PUSH Inc., Toronto, Canada). Before each visit to the laboratory, participants were instructed to refrain from caffeine for ≥ 12 hours and strenuous physical activity for ≥ 24 hours.

Subjects

Twenty-nine professional male youth rugby league players (age: 18 ± 1 years [range: 16 to 19 years]; height: 1.73 ± 0.83 m; body mass: 87.3 ± 20.8 kg) from an English Super League club's academy volunteered to participate in this study. Players reported engaging in structured resistance training 4.3 ± 0.5 times per week for 3.1 ± 1.3 years before the commencement of the study. Player strength characteristics are presented in Table 1. All participants were informed of the experimental procedures to be undertaken prior to signing an institutionally approved informed consent document to participate in the study. Parental or guardian signed consent was also obtained for participants aged < 18 years. Ethical approval for the study was granted by the Sports, Health and Exercise Science Ethics Committee at the University of Hull.

[INSERT TABLE 1 ABOUT HERE]

Procedures

1RM testing

1RM testing was consistent with recognised guidelines established by the National Strength and Conditioning Association (18). A UKSCA accredited S&C coach and a Certified Strength and Conditioning Specialist (CSCS) were present at all testing sessions to ensure correct technique and adherence to the 1RM protocol. For the back squat, an Olympic barbell was placed on the trapezius in a high-bar position. With their feet externally rotated $5\text{--}10^\circ$ and placed shoulder-width apart, participants started in an upright bipedal position and descended downwards until the top of the thigh was at least parallel to the floor before returning to the starting position. Participants were required to maintain constant downward pressure on the barbell (13) and keep their feet in contact with the floor during all repetitions. Bench press

1RM testing was performed on a solid flat bench secured in position inside an adjustable power rack (Perform Better Ltd, Southam, UK). The position of the bench was individually adjusted so that the vertical trajectory of the barbell was in line with participants' intermammary line. Participants unracked the barbell using a self-selected grip width and lay supine on the bench with their arms fully extended. Upon verbal command, participants lowered the barbell until the chest was briefly touched, approximately 3 cm superior to the xiphoid process, before executing full elbow extension. The attempt was considered successful if the participant's head, upper back, and buttocks remained firmly placed on the bench and both feet stayed flat on the floor. The barbell was not permitted to bounce off the chest. Participants performed the eccentric phase of both exercises in a controlled manner at a self-selected velocity and completed the concentric phase as fast as possible.

Test-retest sessions

All test and retest sessions were conducted at the same time of day (7 a.m.) and were separated by seven days. Following a standardised warm-up protocol, participants completed three consecutive repetitions at loads of 20%, 40%, 60% and 80% of 1RM, and two repetitions at 90% of 1RM. These loads were chosen to represent the full loading spectrum and to aid comparisons with previous studies (5, 6). Three minutes of passive rest were provided between different loading conditions and participants were verbally encouraged to execute each repetition with maximal concentric velocity. Additional repetitions were performed if technical lifting requirements were not met or submaximal effort was used, as determined by a consensus from the UKSCA accredited S&C coach and CSCS. GYM was considered the criterion in this study because the device has previously been shown to accurately assess velocity and power in the back squat (6) and bench press (15).

Data analysis

GYM is a commercially available LPT consisting of a floor unit, made up of a steel cable that is wound on a cylindrical spool coupled to the shaft of an optical encoder (15). The floor unit was placed on the floor perpendicular to the right collar of the barbell. In line with manufacturer's instructions, the other end of the cable was vertically attached to the barbell (immediately proximal to the right collar) using a Velcro strap. GYM measures the vertical displacement of its cable in response to changes in barbell position. The displacement data were time-stamped at 20 millisecond time points and down-sampled to 50 Hz for analysis. The sampled data were not filtered. Instantaneous velocity was determined as the change in barbell position with respect to time. Acceleration data were calculated as the change in barbell velocity over the change in time for each consecutive data point. Instantaneous force was determined by multiplying the system mass with acceleration, where system mass was the barbell load plus the relative body mass of the participant (6). Power was then calculated as the product of force and velocity. Data obtained from GYM were transmitted via Bluetooth to a tablet (iPad, Apple Inc., California, USA) using the GymAware v2.1.1 app.

PUSHTM is a wearable inertial sensor consisting of a 3-axis accelerometer and a gyroscope that provides six degrees in its coordinate system. The device was worn on the participant's right forearm, 1-2 cm distal to the elbow crease, with the main button located proximally as per manufacturer's instruction. The acceleration data were smoothed using a Butterworth filter, and vertical velocity was calculated by the integration of acceleration with respect to time. Similarly to GYM, instantaneous force was calculated as the product of acceleration and the system mass, and power was determined by multiplying force with velocity. Data obtained from PUSHTM were recorded at a sampling rate of 200 Hz and transmitted to the PUSHTM v3.1.2 app via a Bluetooth connection with a tablet. PUSHTM and GYM do not require calibration processes.

The participant's body mass and the barbell load used were entered into both apps prior to each repetition. Values of MV and MP obtained by the PUSHTM and GYM were determined as the average of all the instantaneous data collected during the concentric phase of each repetition. PV and PP were calculated as the maximum value registered during the same concentric period. The maximum value of each set of repetitions performed at each load (fastest mean concentric velocity as determined by GYM) was used for analysis.

Statistical analysis

All data were analysed using custom-designed Microsoft Excel spreadsheets (Microsoft Corporation, Redmond, Washington, USA) (24). The concurrent validity and test-retest reliability of PUSHTM were determined by examining each relative load separately (i.e. 20%, 40%, 60%, 80%, and 90% of 1RM). Validity of PUSHTM was assessed using the Pearson product-moment correlation coefficient (Pearson's r) and mean bias with 95% limits of agreement (95% LOA). The standardised mean bias was rated as: trivial (<0.2), small, (0.2 to 0.59), moderate (0.6 to 1.19), large (1.2 to 1.99), very large (2.0 to 3.99) and extremely large (≥ 4.0) (24). Relative reliability was determined using the intraclass correlation coefficient (ICC). Absolute reliability was examined using the standard error of measurement (SEM) and the smallest worthwhile change (SWC). SEM was calculated using the formula $SD_{diff}/\sqrt{2}$ (22) and was also expressed as a percentage of the mean (SEM%). The SWC was calculated as the between-subject SD multiplied by 0.2 (22). The following criteria were used to interpret the strength of the Pearson's r used to assess validity and the ICC estimates used to assess reliability: poor (<0.5), moderate (0.50 to 0.74), good (0.75 to 0.89) and excellent (≥ 0.9) (27). The level for all confidence intervals (CI) was set at 95%.

RESULTS

Figure 1 presents velocity and power data across each relative intensity. The reliability (ICC, SEM%) of MV measurements obtained by GYM ranged from 0.72 to 0.87 and 3.9 to 9.9%, respectively.

[INSERT FIGURE 1 ABOUT HERE]

[INSERT TABLE 2 ABOUT HERE]

Back squat

The standardised mean bias showed small differences between PUSHTM and GYM devices for the measurement of PV and MP at 20% of 1RM. There were moderate to very large underestimations of all other criterion variables (see Table, Supplemental Digital Content 1), which were also evidenced by the 95% LOA (Figures 2 to 5). Despite the evidence of systematic bias, good to excellent correlations ($r \geq 0.75$) were found between PUSHTM and GYM methods for MP and PP measurements at loads of 20% to 80% of 1RM. Good correlations were also found for MV at 20%, 60%, and 80% of 1RM, and PV at 20% and 80% of 1RM.

PUSHTM only demonstrated good reliability for the measurement of MP (ICC = 0.83, 95% CI: 0.66 to 0.91) and PP (ICC = 0.80, 95% CI: 0.62 to 0.90) at 20% of 1RM. The SEM% and ICC estimates tended to worsen as the relative intensity increased (Figures 2 to 5). Absolute SEM and SWC data for all measurements obtained by PUSHTM are presented in Table 2.

Bench press

The standardised mean bias showed that there were no obvious under- or over-estimations of PV at 60% to 90% of 1RM and MP at 60% of 1RM. Small systematic biases were evident for the measurements of MV at 60% of 1RM, PV and MP at 20% and 40% of 1RM, and PP at 90% of 1RM. There were moderate differences between PUSHTM and GYM for all other criterion

variables (see Table, Supplemental Digital Content 1). Good correlations between PUSHTM and GYM were found for the measurement of MV at 40% of 1RM ($r = 0.84$, 95% CI: 0.68 to 0.92), and for MP at 40% ($r = 0.89$, 95% CI: 0.77 to 0.95) and 80% ($r = 0.76$, 95% CI: 0.53 to 0.88) of 1RM.

PUSHTM only showed good reliability for the measurement of MP (ICC = 0.83, 95% CI: 0.67 to 0.92) and PP (ICC = 0.88, 95% CI: 0.76 to 0.94) at 40% of 1RM.

[INSERT FIGURE 2 ABOUT HERE]

[INSERT FIGURE 3 ABOUT HERE]

[INSERT FIGURE 4 ABOUT HERE]

[INSERT FIGURE 5 ABOUT HERE]

DISCUSSION

This study examined the validity and reliability of a wearable inertial sensor (PUSHTM) to measure velocity and power in the back squat and bench press. Our data are the first to demonstrate that the reliability and validity of PUSHTM are contingent on the exercise and the external load lifted. The device was reliable and valid for the measurements of MP at 20% of 1RM in the back squat. In the bench press, PUSHTM provided a reliable and valid measurement of MP at 40% of 1RM.

This study is the first to determine the test-retest reliability of PUSHTM. In the free-weight back squat, there was evidence of good reliability for the measurement of MP (ICC = 0.83, 95% CI: 0.66 to 0.91) and PP (ICC = 0.80, 95% CI: 0.62 to 0.90) at 20% of 1RM. The 95% CIs of these ICC estimates suggest that the true reliability for this population likely ranges from moderate to excellent. Interestingly though, our data demonstrated that the reliability of the device tended

to decrease as the external load increased, as evidenced by both the SEM% and ICC data (Figures 2 to 5). This finding aligns well with a recent study (8) reporting a trend of greater between-subject variation in MV and MP with increasing relative intensities in the back squat. This inverse relationship between reliability and intensity may be attributed to alterations in lower body kinematics with increasing loads. Kellis and colleagues (25) reported a 16° increase in forward trunk inclination between 40-70% of 1RM in the free-weight back squat. Hay and colleagues (20) also found that the absolute angle of the hip increased significantly by 22° when the external load was increased from 40% to 80% of 4RM, possibly due to greater involvement of the hip musculature and a concomitant reduction in knee extensor torque (20). Although technique and squat depth were vigilantly monitored throughout testing, this intrinsic change in lower body kinematics would conceivably alter the pathway and orientation of the inertial sensor during the squat movement. Similarly, in the bench press, horizontal displacement of the barbell has been shown to significantly increase from 86 ± 36 mm at 70% of 1RM to 123 ± 38 mm at 100% of 1RM (28). Greater horizontal displacement of the barbell at heavier loads may result from an increased effort to reduce the moment arm about the shoulder axis (16, 28), which would alter the position of the forearm relative to the barbell during the concentric phase. Caution should therefore be taken when measuring velocity and power at heavier loads in free-weight resistance exercises.

We have provided absolute measures of reliability to enable practitioners to interpret whether training-induced changes in velocity and/or power are practically significant. The SEM represents the typical variation in performance from repeated trials and displays measurement error in the same units as the original measurement (22). It is important for coaches to minimise the SEM in order to detect subtle yet meaningful changes in performance. Sánchez-Medina et al. (34) have eloquently shown that differences in MV between each 5% increment in relative load vary between 0.05 and 0.10 m·s⁻¹ in the back squat. Their data also show that for each 10%

increase in load, the concomitant change in MV varies between 0.11 and 0.18 m·s⁻¹ (34). Based on the SEM values for MV reported in this study (Table 2), the inertial sensor appears reliable enough to detect 10%, but not 5%, changes in relative load. S&C practitioners must judge whether the magnitude of measurement error is acceptable based on the specific needs of their athletes. Clearly, an appropriate balance must be struck between usability, cost, practicality, and reliability of the testing method.

Two previous studies have supported the use of PUSHTM to accurately measure movement velocity during resistance training. Sato and colleagues (35) reported good correlations between PUSHTM and a 3D motion analysis capture system for the measurement of MV and PV in the dumbbell biceps curl (MV: $r = 0.86$; PV: $r = 0.80$) and shoulder press (MV: $r = 0.88$; PV: $r = 0.92$). Using a LPT as the criterion measure, Balsalobre-Fernández and colleagues (5) also suggested that PUSHTM was highly valid at measuring MV ($r = 0.85$) and PV ($r = 0.91$) in the Smith machine back squat. Unlike the free-weight back squat though, the Smith machine restricts barbell displacement to a fixed linear path, which eliminates measurement error resulting from extraneous horizontal motion (12). Furthermore, the Pearson correlation analyses employed in both studies (5, 35) involved combining all repetitions performed by each individual. For example, participants in the Balsalobre-Fernández et al. (5) study performed three repetitions at loads of 20, 40, 50, 60 and 70kg, with each repetition used in the validity analyses. Therefore, all participants provided 15 data points in each paired sample. This technique violates the assumption of independence in the Pearson correlation analysis and is likely to produce erroneous results (4).

To satisfy the assumption of independence, we analysed each relative load separately using the fastest repetition at each load. Our data demonstrated good to excellent correlations between PUSHTM and GYM for MP and PP measurements at loads of 20% to 80% of 1RM. We also found good correlations for measurements of MV at 20%, 60% and 80% of 1RM and for PV

at 20% and 80% of 1RM. Similarly, Banyard and colleagues (6) recently reported that PUSHTM was highly valid for the measurement of MV at light to moderate loads (i.e. <60% of 1RM) and for measuring PV at light loads (i.e. 20% of 1RM). However, they considered all MP and PP data obtained by PUSHTM to be invalid. Differences between these results and our data are readily explained by the different validity criteria used. We employed Pearson's *r* to determine thresholds of acceptable validity, whereas Banyard and colleague's (6) included Pearson's *r*, coefficient of variation (CV) and the effect size in their validity criteria. Interestingly, if the CV was not used in their (6) analyses, the validity of PUSHTM to measure MP and PP would have been considered high for all loads except for 90% and 100% of 1RM (i.e. the same results as the present study). Although the CV is commonly used to assess the validity of variables pertinent to sports medicine (3), it has been suggested that this statistic may be more representative of variability within an individual, rather than within a sample of individuals (30). This appears logical given the CV can only be directly calculated from repeated measurements on a single case (32). Additional differences between studies include the criterion measure used, the number of repetitions performed per load, and the sample population (and therefore the sample heterogeneity).

Though the inertial sensor was valid and reliable for measuring MP at 20% of 1RM in the back squat, the practical applications of prescribing this load are questionable. We instructed participants to keep their feet in contact with the floor during all repetitions in order to standardise technique between each load. Due to the inherent limitation of applying maximal force to the ground when using light loads in the back squat (34), it may be more appropriate for athletes to jump off the ground with 20% of 1RM. Indeed, peak power output in the jump squat has been shown to be approximately twofold greater compared with the back squat (13). Lighter loads ($\leq 30\%$ of 1RM) also elicit the highest PP output in the jump squat exercise (36).

Therefore, further research should evaluate the validity and reliability of inertial sensors to measure power in the jump squat.

In agreement with previous reports (5), we found evidence of systematic bias between the inertial sensor and LPT in the back squat. Specifically, the standardised mean bias showed moderate to very large underestimations of most criterion variables, which were also evidenced by the 95% LOA. This bias is likely underpinned by differences in calculation techniques.

GYM is a portable LPT that directly measures the vertical displacement of its cable. Movement velocity and power output are calculated as derivatives of the displacement data through double differentiation processes. Conversely, the inertial sensor is worn on the forearm and encompasses a 3-axis accelerometer with a gyroscope. Differentiation of the acceleration data then permits the calculation of velocity and power. The differentiation procedures used by both systems, although based on well-established mathematical principles, require extensive data manipulation and therefore result in the amplification of noise and the consequential risk of erroneous data (12). Inertial sensors and LPTs also use different sampling frequencies and methods to correct for motion in the horizontal plane, which may further contribute to the systematic bias. The lack of agreement between PUSHTM and GYM suggests that S&C practitioners should not use these two devices interchangeably and should take caution when comparing data obtained by inertial sensors to normative data obtained by LPTs in the literature.

The inertial sensor showed good reliability for the measurement of MP (ICC = 0.83, 95% CI: 0.67 to 0.92) and PP (ICC = 0.88, 95% CI: 0.76 to 0.94) at 40% of 1RM in the bench press. In addition, a good correlation between PUSHTM and GYM was found at 40% of 1RM for the measurement of MP ($r = 0.89$, 95% CI 0.77 to 0.95), with the lower 95% CI of the Pearson correlation also exceeding the threshold for good validity. Furthermore, the mean bias with 95% LOA for this measurement were relatively narrow (32.3 ± 95.3 W), with the standardised mean bias demonstrating only a small underestimation (0.31) compared to GYM. Therefore, these

data suggest that PUSHTM provides a reliable and valid measurement of MP at 40% of 1RM. It is important to note that maximal MP and PP output were also achieved at 40% of 1RM (Figure 1), which is in agreement with previous research demonstrating that power production in the bench press is optimised at moderate loads (37). This finding indicates that S&C coaches are able to prescribe 40% of 1RM in the bench press to accurately quantify and develop the power-generating capabilities of their athletes.

The criteria for ICC estimates of reliability used in this study were based on recent guidelines for selecting and reporting ICCs (27). For example, an ICC estimate of 0.75 or above was considered a good level of reliability. We also used the same thresholds for Pearson correlations to improve clarity in the interpretation of our data. Many studies (19, 31, 38, 39) have used a correlation threshold of ≥ 0.50 to denote a strong level of validity and/or reliability based on criteria put forward by Cohen (9) and Hopkins (23). On the other hand, some authors have chosen an analytic goal of r being above 0.70 (6, 7). We have provided mean estimates with 95% CIs for all correlation coefficients to enable the reader to make their own interpretation of the data.

In conclusion, these data show that the reliability and validity of the inertial sensor are contingent on the exercise and the external load lifted. The PUSHTM device was reliable and valid for the measurement of MP at light relative loads (e.g. 20% of 1RM) in the back squat. However, the practical applications of using this load are questionable because of the intrinsic limitation of applying maximal force to the ground when lifting light loads in the back squat. In the bench press, PUSHTM obtained a valid and reliable measurement of MP at 40% of 1RM, although a small systematic bias between PUSHTM and GYM devices was present. Practitioners must be cognisant of the measurement error when evaluating changes in performance between repeated trials.

PRACTICAL APPLICATIONS

Though the inertial sensor was considered valid and reliable for measuring MP at 20% of 1RM in the back squat, it may be more appropriate for athletes to jump off the ground with this load in order to optimise power output. Further research should therefore evaluate the validity and reliability of inertial sensors to measure power in the jump squat exercise. Measuring MP at 40% of 1RM provides S&C coaches with a reliable and valid measurement of power output in the bench press. However, inertial sensors and LPTs should not be used interchangeably because of the systematic bias between the two systems. Practitioners should acknowledge the magnitude of measurement error between repeated trials when using inertial sensor technology to quantify velocity and power in resistance training exercises.

References

1. Aarts E, Verhage M, Veenvliet JV, Dolan CV, van der Sluis S. A solution to dependency: using multilevel analysis to accommodate nested data. *Nat Neurosci.* 2014;17(4):491-6.
2. Abernethy P, Wilson G, Logan P. Strength and power assessment. Issues, controversies and challenges. *Sports Med.* 1995;19(6):401-17.
3. Atkinson G, Nevill AM. Statistical methods for assessing measurement error (reliability) in variables relevant to sports medicine. *Sports Med.* 1998;26(4):217-38.
4. Bakdash JZ, Marusich LR. Repeated Measures Correlation. *Front Psychol.* 2017;8:456.
5. Balsalobre-Fernandez C, Kuzdub M, Poveda-Ortiz P, Campo-Vecino JD. Validity and Reliability of the PUSH Wearable Device to Measure Movement Velocity During the Back Squat Exercise. *J Strength Cond Res.* 2016;30(7):1968-74.
6. Banyard HG, Nosaka K, Sato K, Haff GG. Validity of Various Methods for Determining Velocity, Force and Power in the Back Squat. *Int J Sports Physiol Perform.* 2017;1-25.
7. Bishop D, Spencer M, Duffield R, Lawrence S. The validity of a repeated sprint ability test. *J Sci Med Sport.* 2001;4(1):19-29.
8. Carroll KM, Sato K, Bazylar CD, Triplett NT, Stone MH. Increases in Variation of Barbell Kinematics Are Observed with Increasing Intensity in a Graded Back Squat Test. *Sports.* 2017;5(3):51.
9. Cohen J. *Statistical Power Analysis for the Behavioral Sciences.* New York, NY: Routledge Academic; 1988.
10. Conceicao F, Fernandes J, Lewis M, Gonzalez-Badillo JJ, Jimenez-Reyes P. Movement velocity as a measure of exercise intensity in three lower limb exercises. *J Sports Sci.* 2016;34(12):1099-106.
11. Cormie P, Deane R, McBride JM. Methodological concerns for determining power output in the jump squat. *J Strength Cond Res.* 2007;21(2):424-30.
12. Cormie P, McBride JM, McCaulley GO. Validation of power measurement techniques in dynamic lower body resistance exercises. *J Appl Biomech.* 2007;23(2):103-18.
13. Cormie P, McCaulley GO, Triplett NT, McBride JM. Optimal loading for maximal power output during lower-body resistance exercises. *Med Sci Sports Exerc.* 2007;39(2):340-9.
14. Crewther BT, Kilduff LP, Cunningham DJ, Cook C, Owen N, Yang GZ. Validating two systems for estimating force and power. *Int J Sports Med.* 2011;32(4):254-8.
15. Drinkwater EJ, Galna B, McKenna MJ, Hunt PH, Pyne DB. Validation of an optical encoder during free weight resistance movements and analysis of bench press sticking point power during fatigue. *J Strength Cond Res.* 2007;21(2):510-7.
16. Elliott BC, Wilson GJ, Kerr GK. A biomechanical analysis of the sticking region in the bench press. *Med Sci Sports Exerc.* 1989;21(4):450-62.
17. Gonzalez-Badillo JJ, Sanchez-Medina L. Movement velocity as a measure of loading intensity in resistance training. *Int J Sports Med.* 2010;31(5):347-52.
18. Haff G, G., Triplett TN. *Essentials of Strength Training and Conditioning.* Champaign, IL: Human Kinetics; 2015.
19. Harper LD, Hunter R, Parker P, Goodall S, Thomas K, Howatson G, et al. Test-Retest Reliability of Physiological and Performance Responses to 120 Minutes of Simulated Soccer Match Play. *J Strength Cond Res.* 2016;30(11):3178-86.
20. Hay JG, Andrews JG, Vaughan CL, Ueya K. Load, speed and equipment effects in strength-training exercises. In: Matsui H, Kobayashi K, editors. *Biomechanics VIII-B.* Champaign, IL: Human Kinetics; 1983. p. 939–50.

21. Hopkins WG, Hawley JA, Burke LM. Design and analysis of research on sport performance enhancement. *Med Sci Sports Exerc.* 1999;31(3):472-85.
22. Hopkins WG. Measures of reliability in sports medicine and science. *Sports Med.* 2000;30(1):1-15.
23. Hopkins WG. A new view of statistics. Internet Society for Sport Science: <http://www.sportsci.org/resource/stats/>. 2000.
24. Hopkins WG. Spreadsheets for analysis of validity and reliability. *Sportscience.* 2015;19:36-42.
25. Kellis E, Arambatzi F, Papadopoulos C. Effects of load on ground reaction force and lower limb kinematics during concentric squats. *J Sports Sci.* 2005;23(10):1045-55.
26. Kenny DA, Judd CM. Consequences of violating the independence assumption in analysis of variance. *Psychol Bull.* 1986;99(3):422-31.
27. Koo TK, Li MY. A Guideline of Selecting and Reporting Intraclass Correlation Coefficients for Reliability Research. *Journal of Chiropractic Medicine.* 2016;15(2):155-63.
28. Krol H, Golas A. Effect of Barbell Weight on the Structure of the Flat Bench Press. *J Strength Cond Res.* 2017;31(5):1321-37.
29. Morán-Navarro R, Martínez-Cava A, Sánchez-Medina L, Mora-Rodríguez R, González-Badillo JJ, Pallarés JG. Movement velocity as a measure of level of effort during resistance exercise. *J Strength Cond Res.* 2017.
30. Quan H, Shih WJ. Assessing reproducibility by the within-subject coefficient of variation with random effects models. *Biometrics.* 1996;52(4):1195-203.
31. Roe G, Darrall-Jones J, Black C, Shaw W, Till K, Jones B. Validity of 10-HZ GPS and Timing Gates for Assessing Maximum Velocity in Professional Rugby Union Players. *Int J Sports Physiol Perform.* 2017;12(6):836-9.
32. Sale DG. Testing strength and power. In: MacDougall JD, Wenger HA, Green HJ, editors. *Physiological testing of the high performance athlete.* Champaign, IL: Human Kinetics; 1991. p. 21-106.
33. Sanchez-Medina L, Gonzalez-Badillo JJ. Velocity loss as an indicator of neuromuscular fatigue during resistance training. *Med Sci Sports Exerc.* 2011;43(9):1725-34.
34. Sánchez-Medina L, Pallarés JG, Pérez CE, Morán-Navarro R, González-Badillo JJ. Estimation of relative load from bar velocity in the full back squat exercise. *Sports Medicine International Open.* 2017;1(02):E80-E8.
35. Sato KK, Beckham G, Carroll K, Bazyler C, Sha Z, Haff GG. Validity of wireless device measuring velocity of resistance exercises. *Journal of Trainology.* 2015;4(1):15-8.
36. Soriano MA, Jimenez-Reyes P, Rhea MR, Marin PJ. The Optimal Load for Maximal Power Production During Lower-Body Resistance Exercises: A Meta-Analysis. *Sports Med.* 2015;45(8):1191-205.
37. Soriano MA, Suchomel TJ, Marin PJ. The Optimal Load for Maximal Power Production During Upper-Body Resistance Exercises: A Meta-Analysis. *Sports Med.* 2017;47(4):757-68.
38. Veugelers KR, Naughton GA, Duncan CS, Burgess DJ, Graham SR. Validity and Reliability of a Submaximal Intermittent Running Test in Elite Australian Football Players. *J Strength Cond Res.* 2016;30(12):3347-53.
39. Weaving D, Whitehead S, Till K, Jones B. Validity of Real-Time Data Generated by a Wearable Microtechnology Device. *J Strength Cond Res.* 2017;31(10):2876-9.
40. Wilson GJ, Newton RU, Murphy AJ, Humphries BJ. The optimal training load for the development of dynamic athletic performance. *Med Sci Sports Exerc.* 1993;25(11):1279-86.

Figure and Table Captions

Table 1. Baseline strength characteristics of study participants.

Table 2. Absolute reliability of the wearable inertial sensor in the back squat and bench press

Figure 1. Values for mean velocity (A and B), peak velocity (C and D), mean power (E and F) and peak power (G and H) in the back squat and bench press. Data are presented as means \pm SD.

Figure 2. Validity and reliability of the wearable inertial sensor to measure mean velocity in the back squat and bench press. Validity was assessed using Pearson product-moment correlation coefficient (A) and the mean bias with 95% limits of agreement (B). Reliability was determined using the intraclass correlation coefficient (C) and standard error of measurement as a percentage of the mean (D). Area shaded in grey represents a good level of validity/reliability. 1RM = one repetition maximum. Data are presented as means \pm 95% confidence intervals.

Figure 3. Validity and reliability of the wearable inertial sensor to measure peak velocity in the back squat and bench press. Validity was assessed using Pearson product-moment correlation coefficient (A) and the mean bias with 95% limits of agreement (B). Reliability was determined using the intraclass correlation coefficient (C) and standard error of measurement as a percentage of the mean (D). Area shaded in grey represents a good level of validity/reliability. 1RM = one repetition maximum. Data are presented as means \pm 95% confidence intervals.

Figure 4. Validity and reliability of the wearable inertial sensor to measure mean power in the back squat and bench press. Validity was assessed using Pearson product-moment correlation coefficient (A) and the mean bias with 95% limits of agreement (B). Reliability was determined using the intraclass correlation coefficient (C) and standard error of measurement as a

percentage of the mean (D). Area shaded in grey represents a good level of validity/reliability.

1RM = one repetition maximum. Data are presented as means \pm 95% confidence intervals.

Figure 5. Validity and reliability of the wearable inertial sensor to measure peak power in the back squat and bench press. Validity was assessed using Pearson product-moment correlation coefficient (A) and the mean bias with 95% limits of agreement (B). Reliability was determined using the intraclass correlation coefficient (C) and standard error of measurement as a percentage of the mean (D). Area shaded in grey represents a good level of validity/reliability.

1RM = one repetition maximum. Data are presented as means \pm 95% confidence intervals.

519 **Supplemental Digital Content 1.** Standardised mean bias between PUSHTM and GYM
520 methods

521 **Table 1.** Baseline strength characteristics of study participants

Back Squat (kg)		Bench Press (kg)	
1RM	Relative 1RM	1RM	Relative 1RM
145.5 ± 24.4	1.71 ± 0.35	100.8 ± 16.4	1.18 ± 0.26



1RM = one repetition maximum; relative 1RM = one repetition maximum normalised to body mass. Data are presented as means ± SD.


Table 2. Absolute reliability of the wearable inertial sensor in the back squat and bench press

		Back Squat					Bench Press				
		20%	40%	60%	80%	90%	20%	40%	60%	80%	90%
MV	SEM	0.08	0.07	0.06	0.06	0.06	0.11	0.08	0.08	0.06	0.05
(m·s⁻¹)	SWC	0.03	0.02	0.02	0.02	0.01	0.03	0.02	0.02	0.02	0.01
PV	SEM	0.12	0.18	0.11	0.11	0.12	0.21	0.11	0.12	0.08	0.10
(m·s⁻¹)	SWC	0.04	0.04	0.03	0.03	0.02	0.05	0.04	0.04	0.02	0.02
MP	SEM	128.3	121.5	105.9	129.5	117.0	70.6	33.8	51.6	51.3	45.7
(W)	SWC	59.1	41.6	32.4	32.9	30.0	19.0	20.3	18.2	15.6	15.5
PP	SEM	261.2	345.8	279.4	345.4	359.5	221.9	151.0	273.0	137.5	131.9
(W)	SWC	112.3	115.6	95.9	80.7	87.5	71.1	84.2	69.2	40.0	40.8

MV = mean velocity; PV = peak velocity; MP = mean power; PP = peak power; SEM = standard error of measurement; SWC

= smallest worthwhile change.


 GYM
  PUSHTM

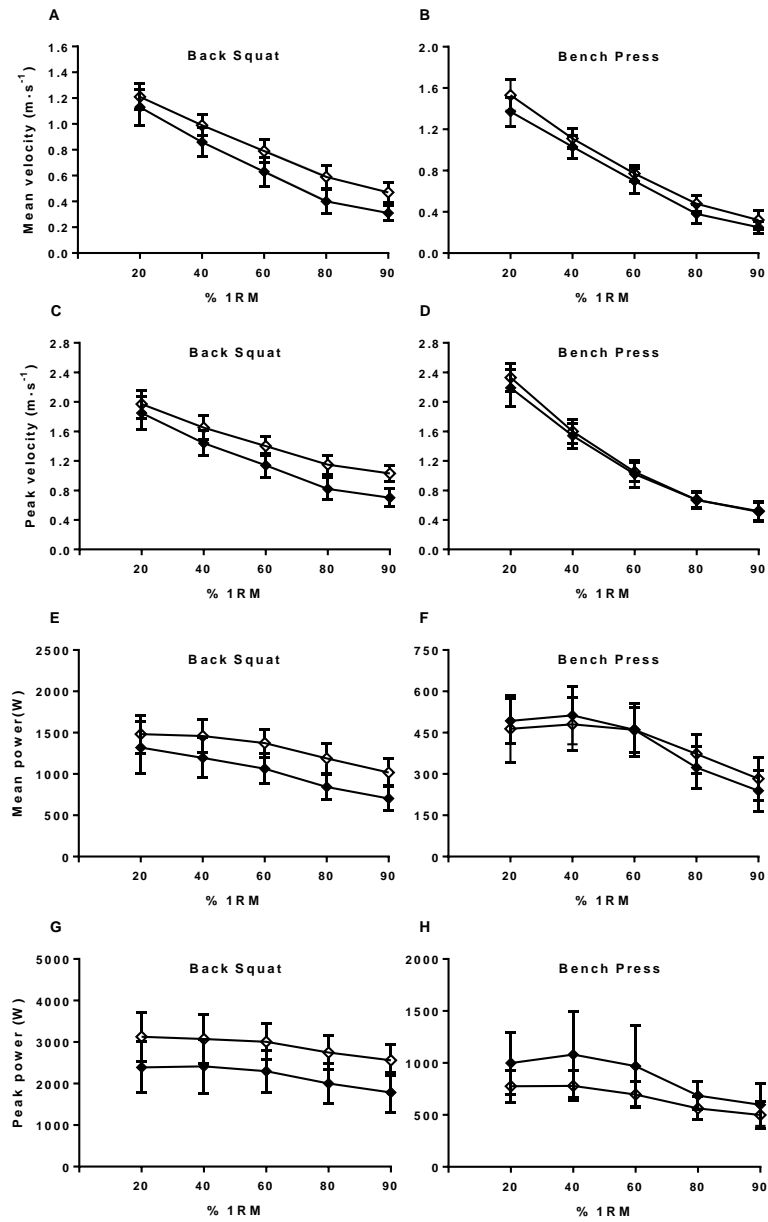

Mean velocity


● Back Squat

□ Bench Press

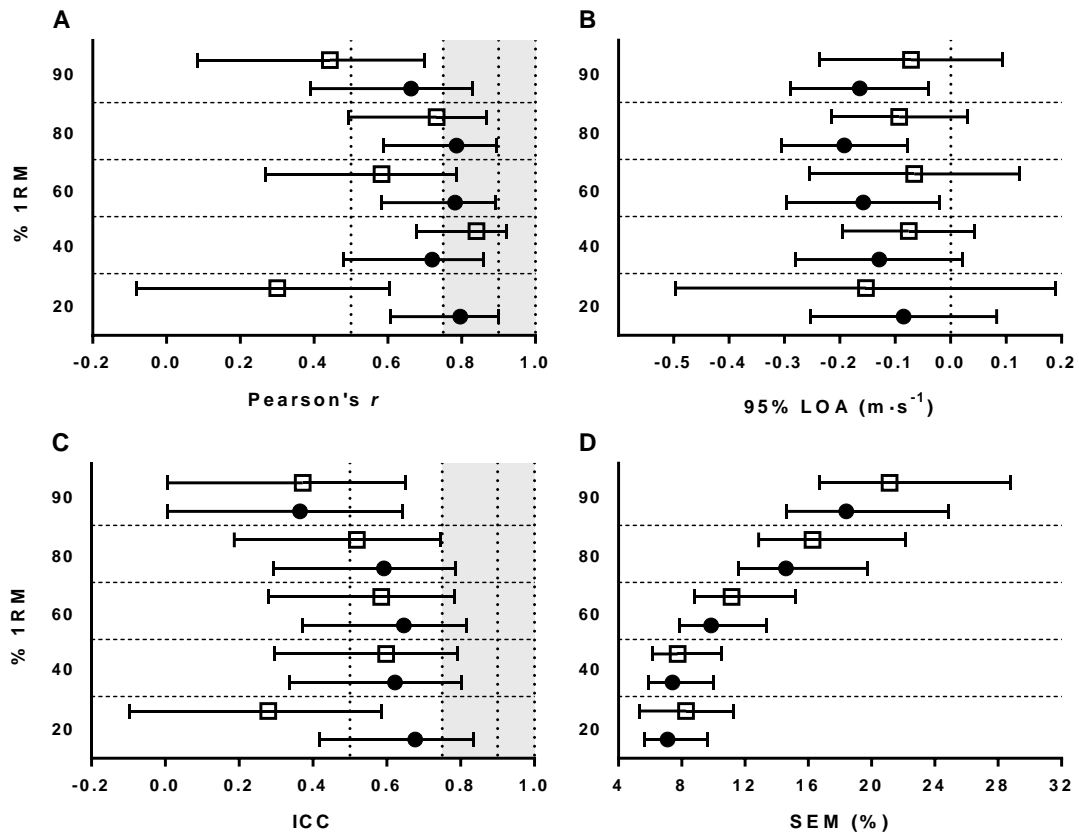

Peak velocity


● Back Squat □ Bench Press

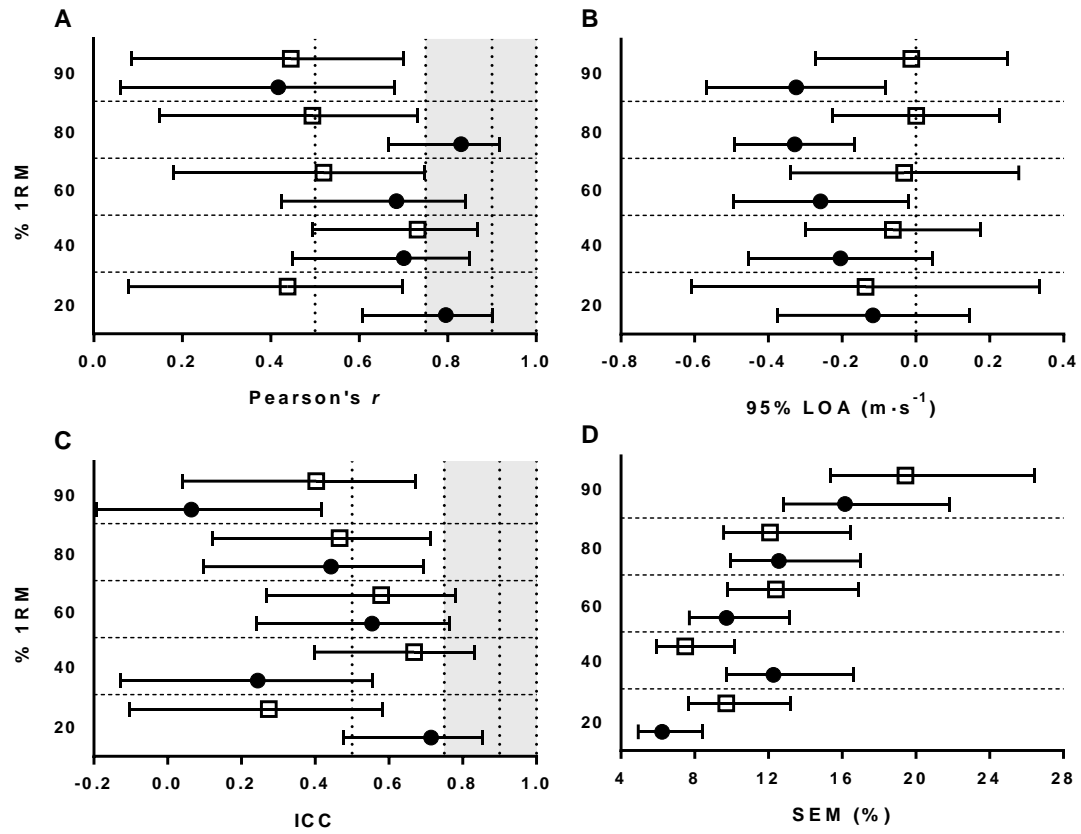

Mean power


● Back Squat

□ Bench Press

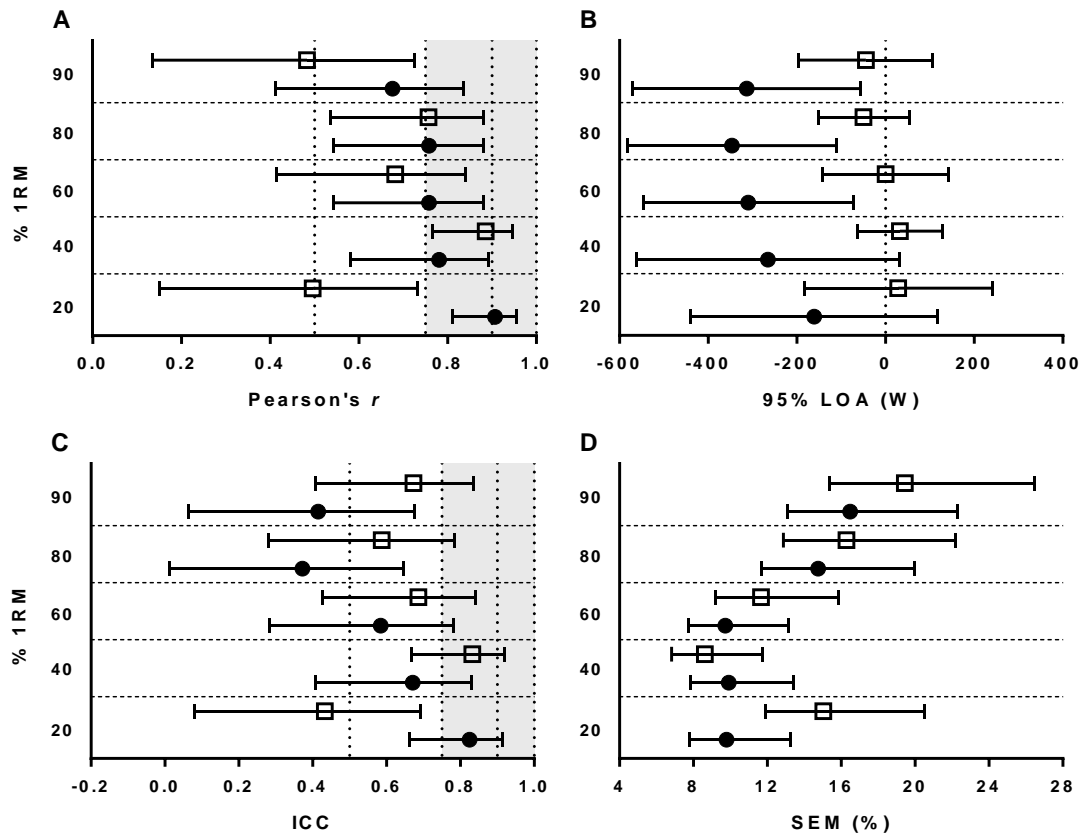

Peak power

● Back Squat □ Bench Press

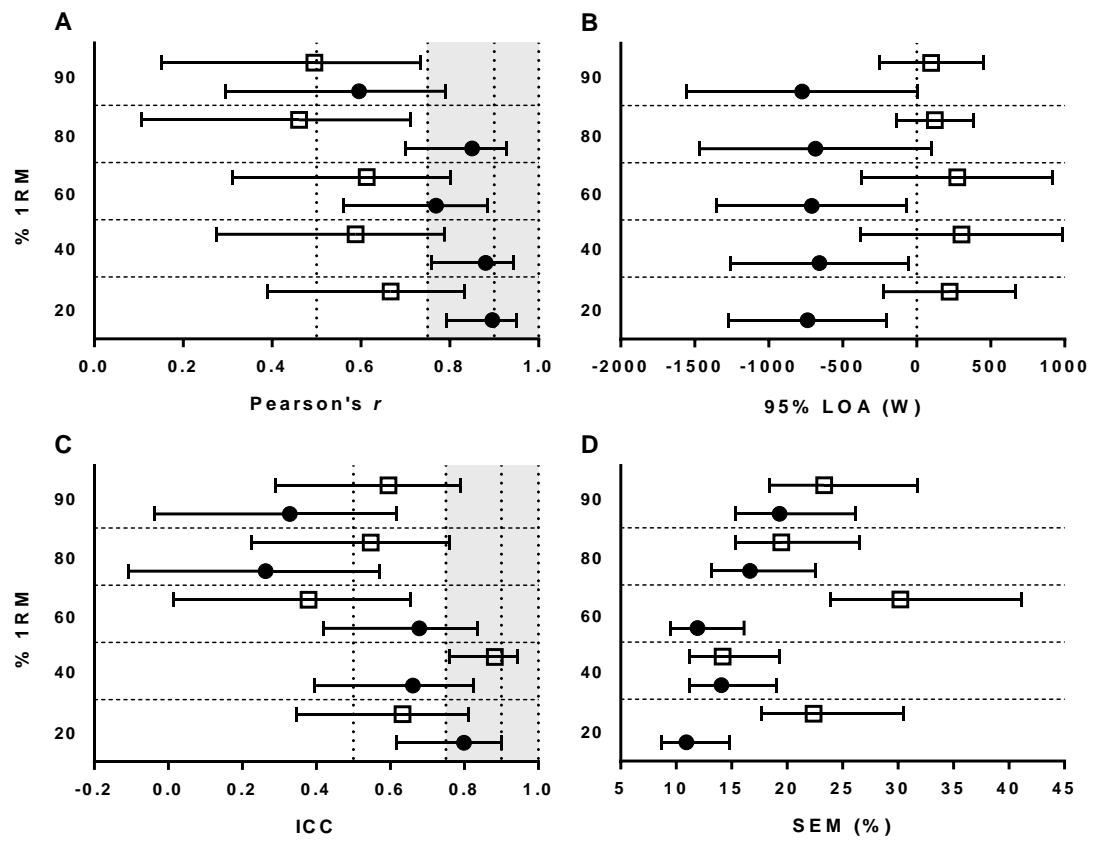

Supplemental Digital Content 1. Standardised mean bias between PUSH™ and GYM methods

	Back Squat					Bench Press				
	20%	40%	60%	80%	90%	20%	40%	60%	80%	90%
MV (m·s ⁻¹)	0.61	1.17	1.41	2.23	2.61	1.06	0.68	0.55	1.03	1.12
PV (m·s ⁻¹)	0.53	1.20	1.58	2.23	2.74	0.55	0.37	0.18	0.00	0.10
MP (W)	0.51	1.10	1.73	2.24	2.08	0.35	0.31	0.00	0.64	0.60
PP (W)	1.20	1.01	1.39	1.43	1.59	0.74	0.73	0.70	0.88	0.48

MV = mean velocity; PV = peak velocity; MP = mean power; PP = peak power. Standardised mean bias of <0.2, 0.2 to 0.59, 0.6 to 1.19, 1.2 to 1.99, 2.0 to 3.99 and ≥4.0 were considered trivial, small, moderate, large, very large and extremely large, respectively.